


# REDUCTION OF AIRBORNE BACTERIA

IN A MALE TOILET

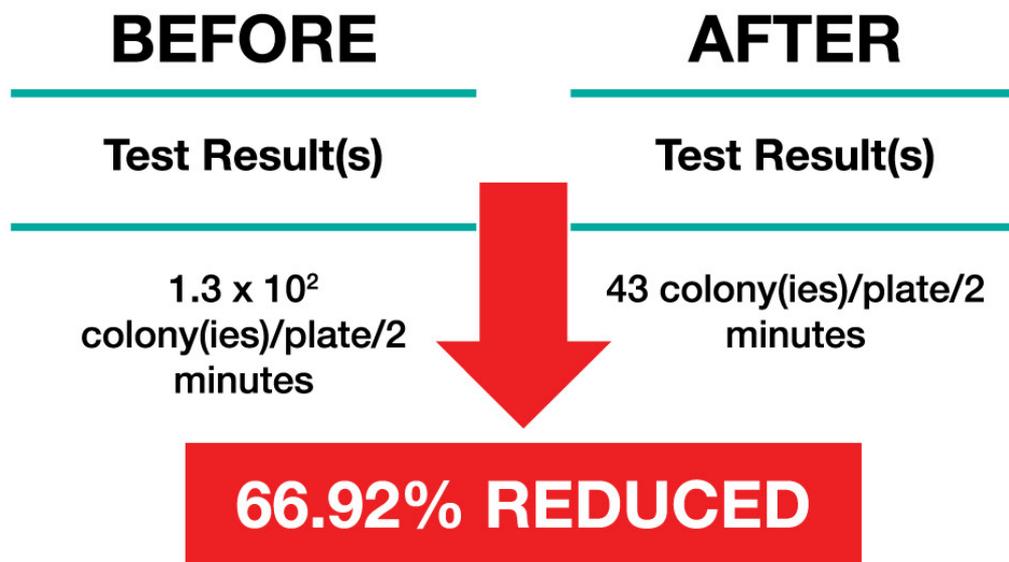

**Field test location:**

A male toilet in Singapore.

**Conducted by:**

Ugene Laboratory, Singapore.

**Test method:**

America Public Health Association, 19th Edition, 1995 - Potato Dextrose Agar @ 25 deg C, 5 days; Air Monitoring - Total Mould Count.

**Test results:**

The Medklinn Air+Surface Sterilizer was very effective at deactivating microbes at ambient condition to approximately 66.92% reduction.